


EM=396

LCMS Scan ESI-

Ret. Time: 3.40

<<<< NEGATIVE SPECTRA >>>>

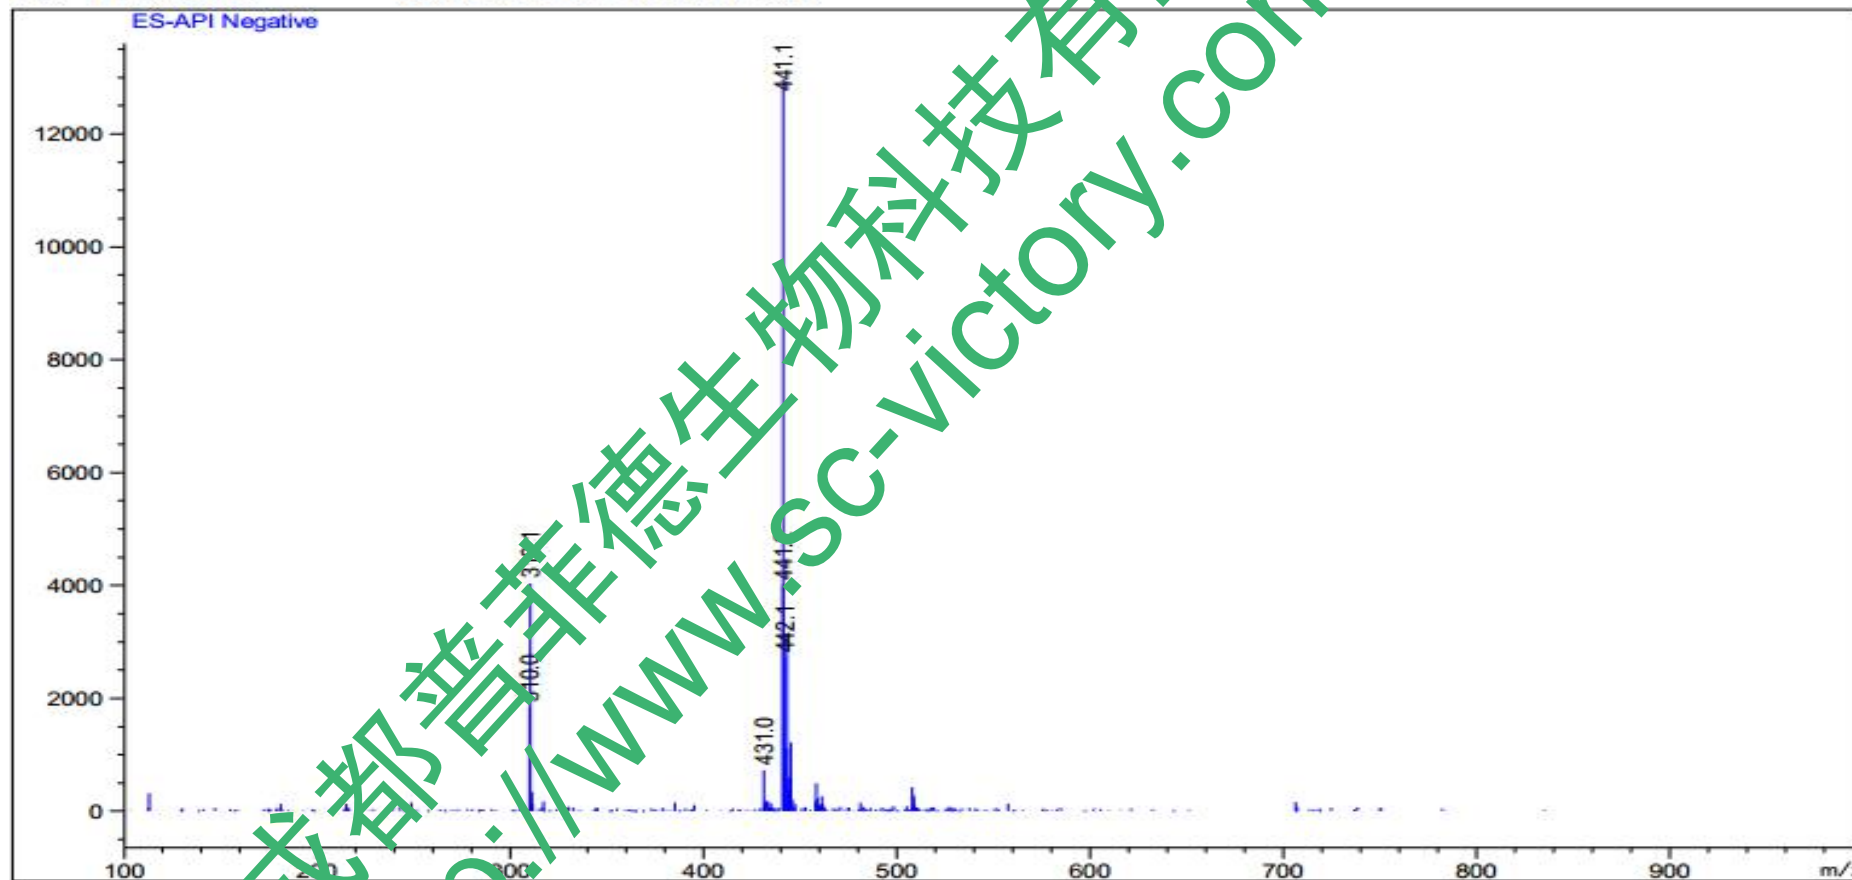

成都普菲德生物科技有限公司
<http://www.SC-victory.com>