


GLP134

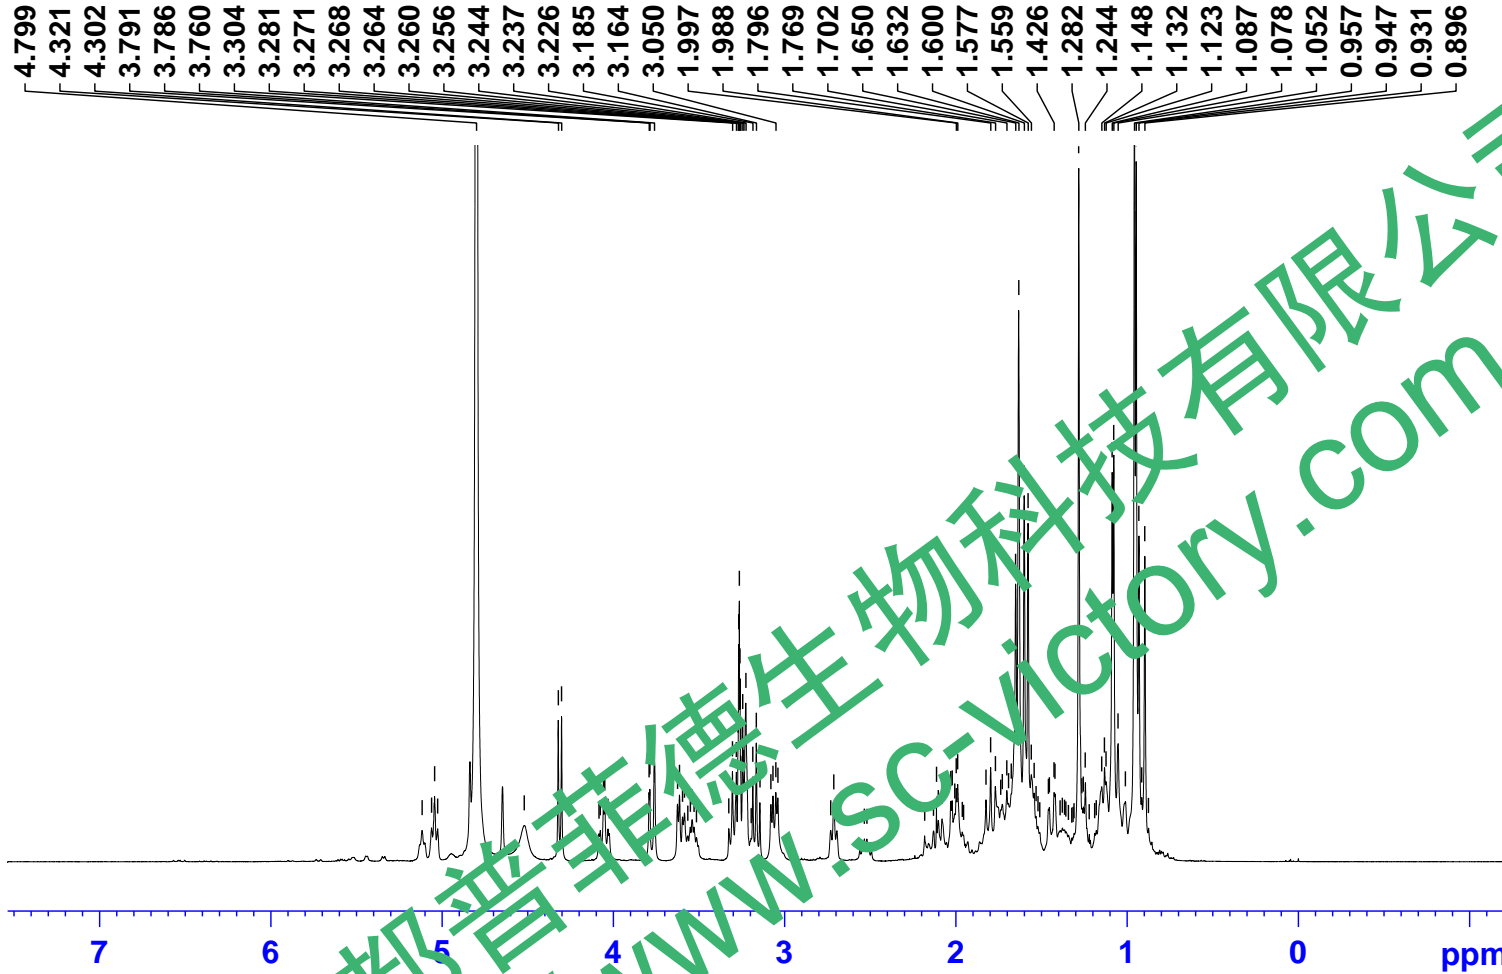

4.799
4.321
4.302
3.791
3.786
3.760
3.304
3.281
3.271
3.268
3.264
3.260
3.256
3.244
3.237
3.226
3.185
3.164
3.050
1.997
1.988
1.796
1.769
1.702
1.650
1.632
1.600
1.577
1.559
1.426
1.282
1.244
1.148
1.132
1.123
1.087
1.078
1.052
0.957
0.947
0.931
0.896

Current Data Parameters
NAME GLP134
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210809
Time 13.18 h
INSTRUM spect
PROBHD Z116098_0564 (
PULPROG zg30
TD 65536
SOLVENT MeOD
NS 16
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 32.03
DW 62.400 usec
DE 6.50 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
P1 10.35 usec
PLW1 14.56099987 W

F2 - Processing parameters
SI 65536
SF 400.1300262 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

1.093
1.786
2.094
0.975
1.000
0.978
1.909
1.056
3.011
1.037
0.997
3.082
12.976
5.973
16.074

成都普菲德生物科技有限公司
http://www.sc-victory.com