

Display Report


Analysis Info

Analysis Name D:\Data\test\0825\yishulisu_16_01_1681.d
Method 1681.m
Sample Name yishulisu
Comment

Operator
Instrument bruker
amaZon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Negative	Alternating Ion Polarity	on
Mass Range Mode	UltraScan	Scan Begin	70 m/z	Scan End	1000 m/z
Capillary Exit	-140.0 V	n/a	n/a	Trap Drive	50.6
Accumulation Time	4377 μ s	Averages	5 Spectra	Auto MS/MS	off

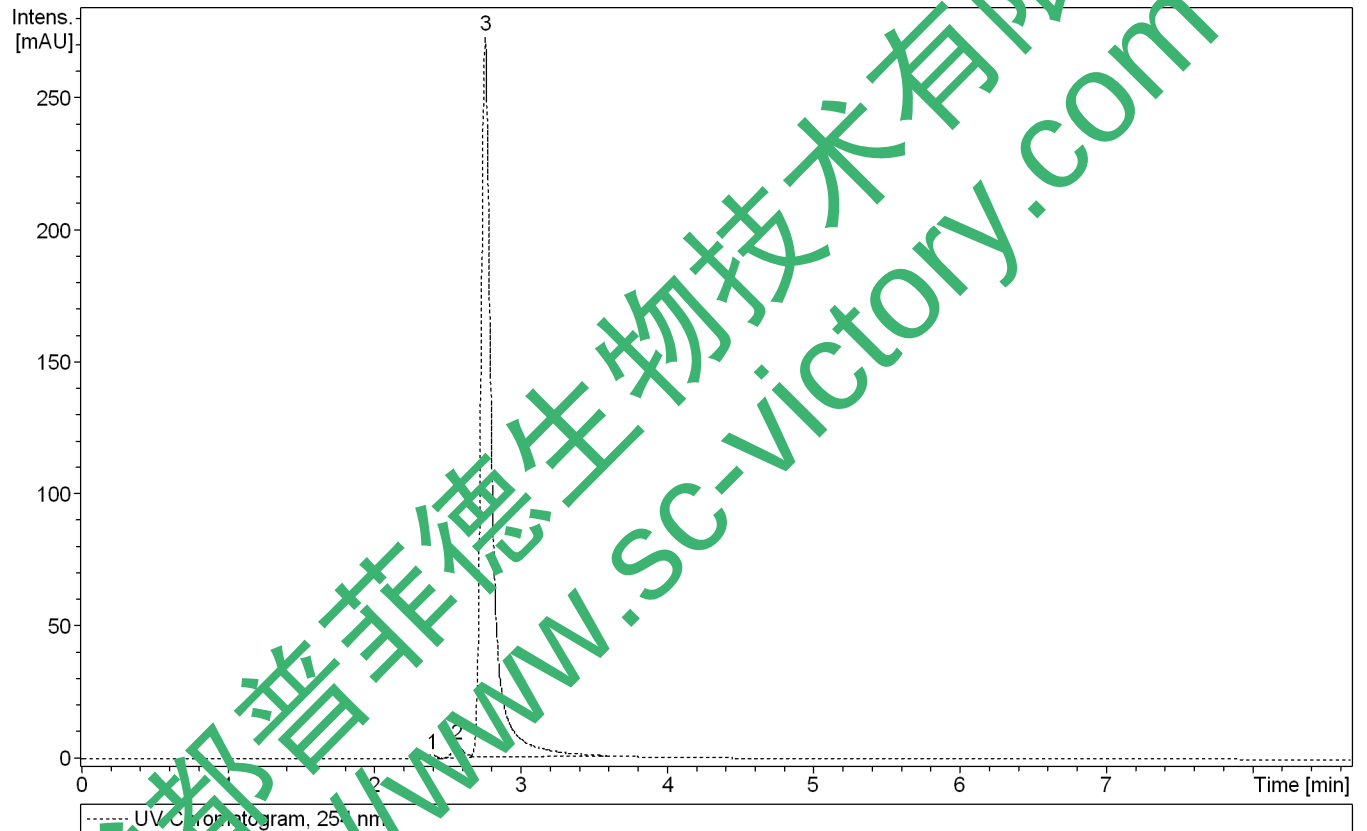

#	RT [min]	Area	Area Frac. %
1	2.4	5.925	0.4
2	2.6	24.382	1.6
3	2.8	1469.012	98.0

Display Report

Analysis Info

Analysis Name D:\Data\test\0825\yishulisu_16_01_1681.d
Method 1681.m
Sample Name yishulisu
Comment

Operator
Instrument bruker
amaZon SL

Acquisition Parameter

Ion Source Type	ESI	Ion Polarity	Negative	Alternating Ion Polarity	on
Mass Range Mode	UltraScan	Scan Begin	70 m/z	Scan End	1000 m/z
Capillary Exit	-140.0 V	n/a	n/a	Trap Drive	50.6
Accumulation Time	4377 μ s	Averages	5 Spectra	Auto MS/MS	off

