



GLP143

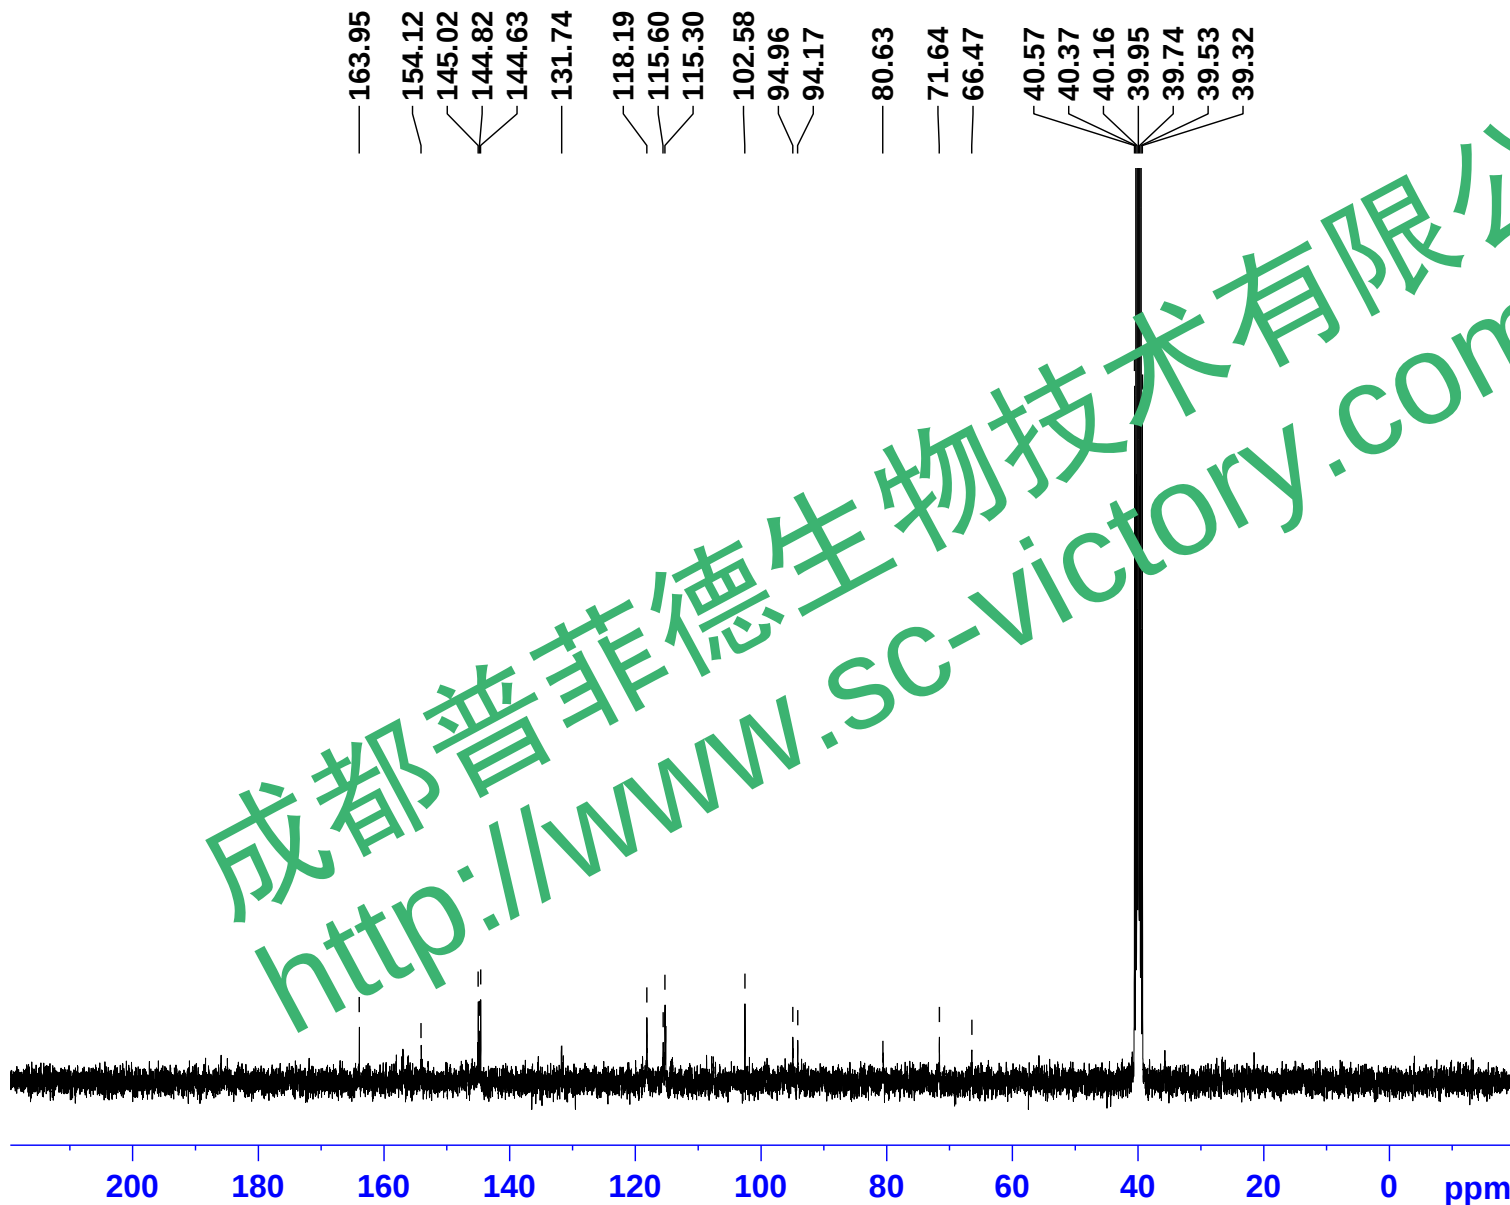

GLP143

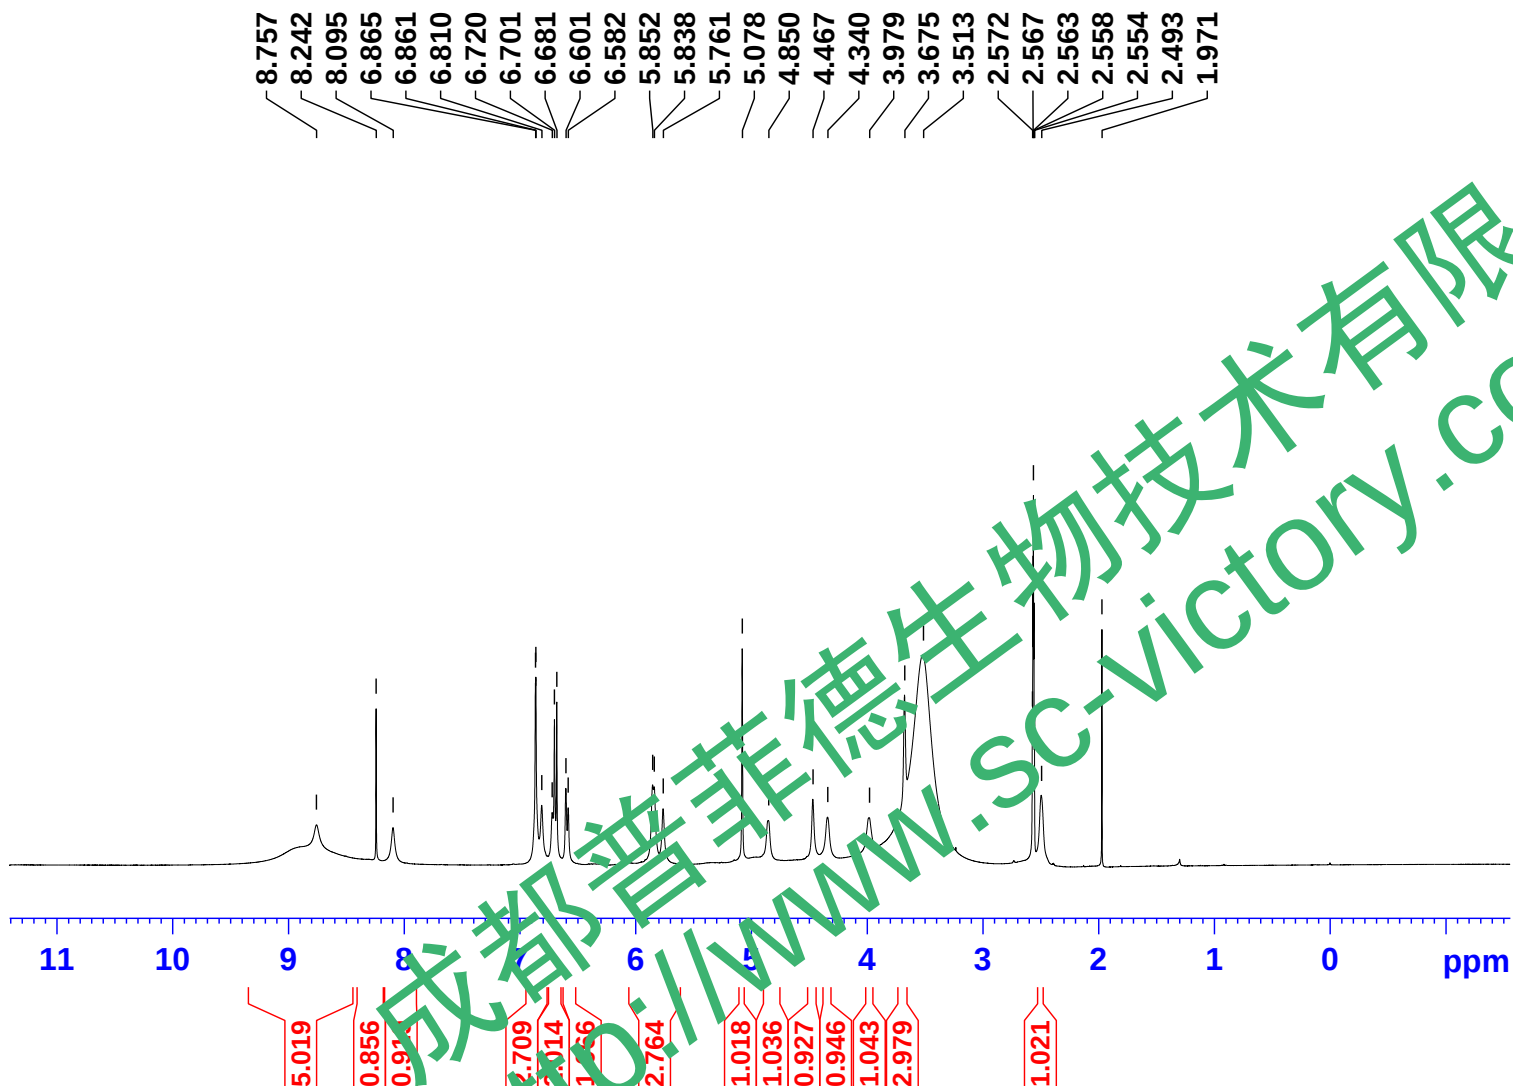

Current Data Parameters
NAME GLP143
EXPNO 10
PROCNO 1

F2 - Acquisition Parameters
Date_ 20210911
Time 9.13 h
INSTRUM spect
PROBHD Z116098_0564 (zg30)
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 186
DS 2
SWH 8012.820 Hz
FIDRES 0.244532 Hz
AQ 4.0894465 sec
RG 70.67
DW 62.400 usec
DE 6.50 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1
SF01 400.1324708 MHz
NUC1 1H
P1 10.35 usec
PLW1 14.56099987 W

F2 - Processing parameters
SI 65536
SF 400.1299786 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00